



BeStar Technologies Inc.

Address: 761 N. 17th Street Unit 4, St. Charles, IL 60174

Tel : 847-261-2850 E-mail : sales@bestartech.com Web : www.bestartech.com

Document Number : 0603-71
Revision : A4
Total Pages : 5
Prepare by : Loki, Lo
Date : 24 September, 2018

SoniCrest Brand Acoustic Components

www.jlsonicrest.com

Document Type : Specification
Product Type : Electro-magnetic Sound Generator Component
Part Number : HCM2606AX

A1 - New issue created by Leo Sin on 30 Mar., 2006		
A2 - Updated RoHS version by Leo Sin on 24 Aug., 2006		
A3 - Updated section 4 - 6 by Loki, Lo on 26 Apr., 2013		
A4 - Updated section 6 by Loki, Lo on 24 Sept., 2018		

This material is the property of BeStar Technologies Inc.
Unauthorized copying or use of this material is prohibited.

1. Purpose and Scope

This document contains both general requirements, qualification requirements, and those specific electrical, mechanical requirements for this part.

2. Description

26 x 26 mm electro-magnetic sound generator with built-in oscillation circuit, RoHS compliant.

3. Application

Computers and Peripherals, Portable Equipment, Automobile Electronics, POS System, Household Appliances, etc.

4. Component Requirement

4.1. General Requirement

4.1.1.	Operating Temperature Range	: -20°C to +60°C
4.1.2.	Storage Temperature Range	: -30°C to +70°C
4.1.3.	Weight	: Approx. 17g
4.1.4.	Housing Material	: ABS

4.2. Electrical Requirement

4.2.1.	Rated Voltage	: 6V
4.2.2.	Operating Voltage	: 4 ~ 8 V
4.2.3.	Rated Current	: <=50mA
4.2.4.	Generated Frequency	: 400 ± 100 Hz
4.2.5.	Sound Pressure Level at 10cm (Applying rated voltage)	: >=95dB

4.3. Mechanical Requirement

4.3.1.	Layout and Dimension	: See Section 6, Figure 3
--------	----------------------	---------------------------

4.4. Test Setup of SPL and Frequency Measurement

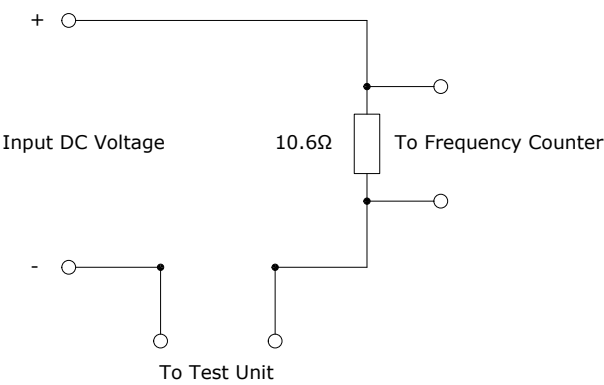


Figure 1. Frequency Testing Circuit

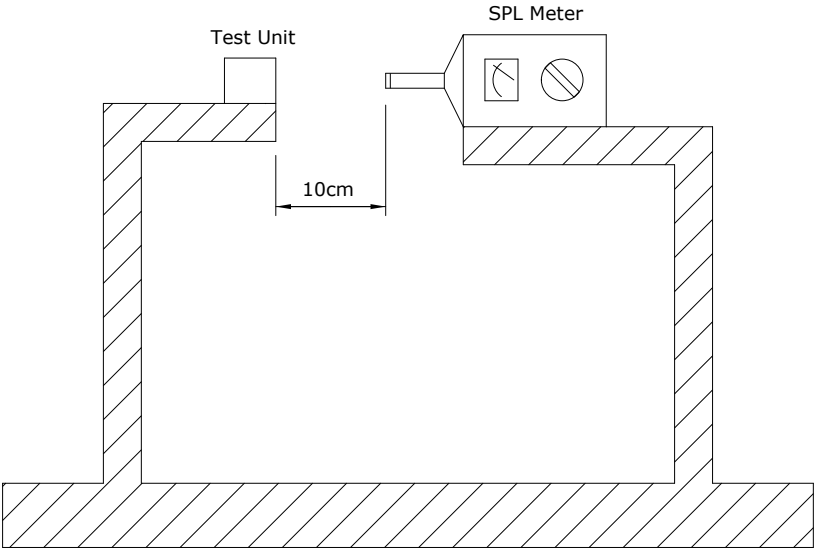


Figure 2. SPL Inspection Test Setup

Notes : Input 6V DC into samples. Measure SPL using a calibrated SPL meter 10cm from the alert port. Sound level meter to be in accordance with IEC651 (1979) Type 1 and/or ANSI S1.4-1983. The meter must be checked on a daily basis using a calibrated acoustic calibrator recommended by the manufacturer. Measurement should be carried out in a free field environment or at least 40cm from any surface.

5. Reliability Test

- 5.1. Operating Life** : Subject samples to room condition for 96 hours with rated voltage. Components must be fully stabilized before data is taken, which may require up to a 2 hours soak.
- 5.2. High Temperature** : Subject samples to +70°C for 72 hours with rated voltage. Components must be fully stabilized at temperature extremes before data is taken, which may require up to a 2 hours soak.
- 5.3. Low Temperature** : Subject samples to -30°C for 72 hours with rated voltage. Components must be fully stabilized at temperature extremes before data is taken, which may require up to a 2 hours soak.
- 5.4. Temperature Shock** : Each temperature cycle shall consist of 30 minutes at -30°C, 15 minutes at +20°C, 30 minutes at +70°C and 15 minutes at +20°C. Test duration is for 10 cycles.
- 5.5. Static Humidity** : Precondition at room temperature for 1 hour. Then expose to +40°C with 90 to 95% relative humidity for 96 hours. Finally dry at room ambient for 2 hours before taking final measurement.
- 5.6. Random Vibration** : Secure samples. Vibrated randomly 10Hz ~ 50Hz with 1.5mm peak amplitude and 1 minutes sweep duration. The test duration is 30 minutes per plane (x, y, z).
- 5.7. Drop Test** : Drop samples naturally from the height of 0.8m onto a wooden board six times.
- 5.8. Solderability** : 235°C±5°C for 2±0.5 seconds.

6. Mechanical Layout

Unit : mm
Tolerance : Linear XX.X = ±0.5
 XX.XX = ±0.05
 Angular = ±0.25°
(unless otherwise specified)

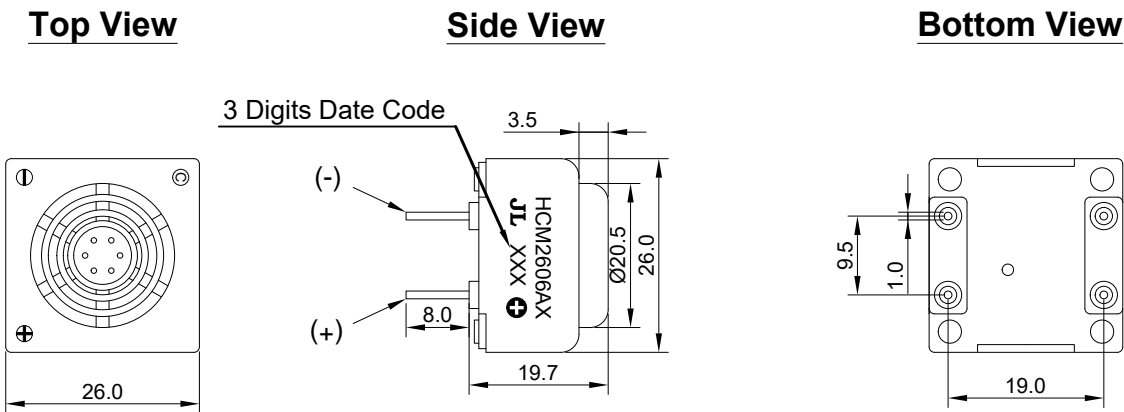


Figure 3. HCM2606AX Mechanical Layout

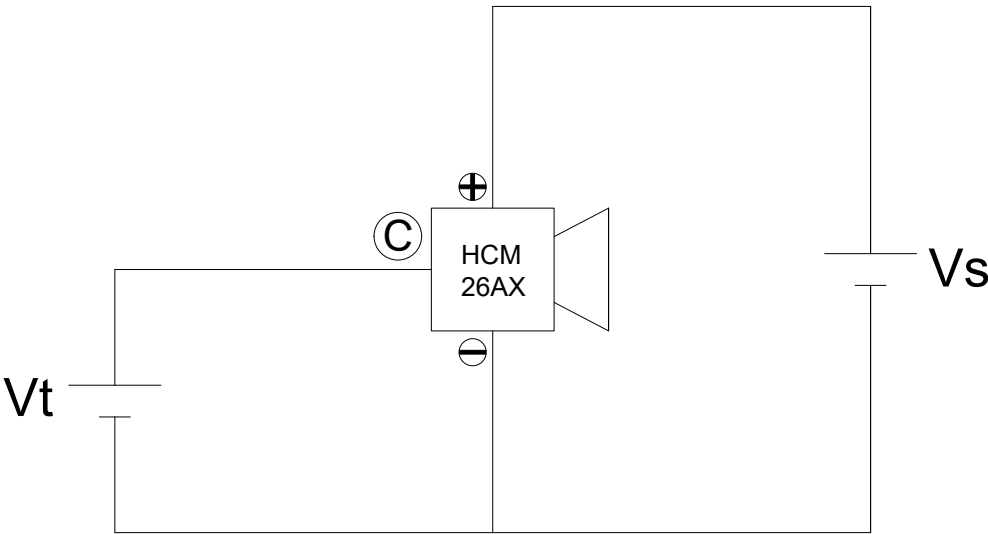


Figure 4. Coupled Circuit